


70-70 ArialI-B 022217


Cytometer: FACSArialI
 Cytometer Name: FACSArialI
 Serial Number: 1
 Input Device: Manual
 Sheath Pressure: 70.00
 Nozzle Size: 70
 Window Extension: 2.00

User: Administrator
 Institution: N/A
 Software: BD FACSDiva 8.0.1
 Date: 5/2/2017 4:55:21 PM


Red Laser (640nm)

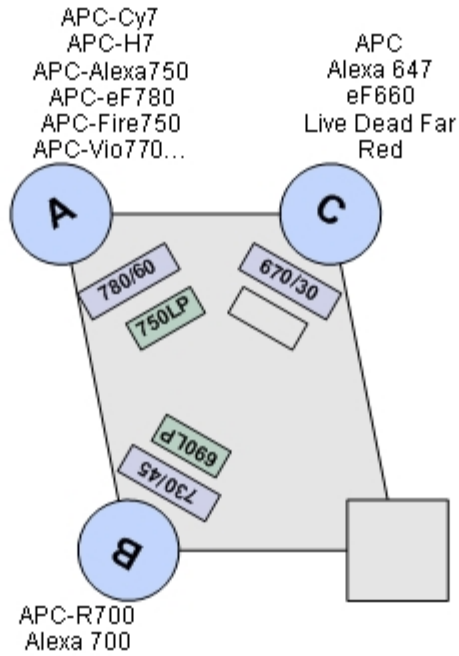


UV Laser (355nm)

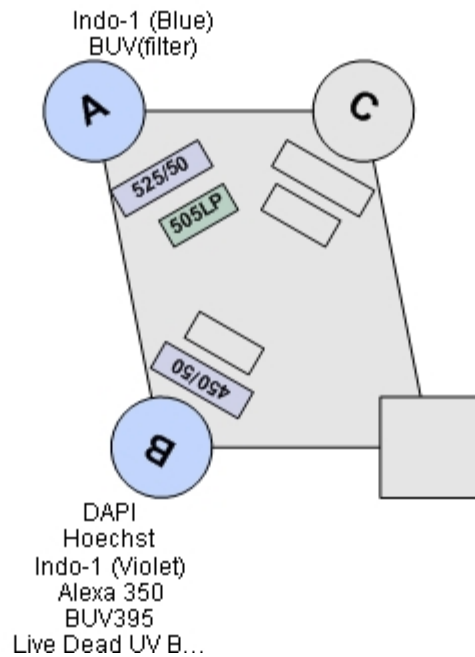


Blue Laser
(488nm)
FSC

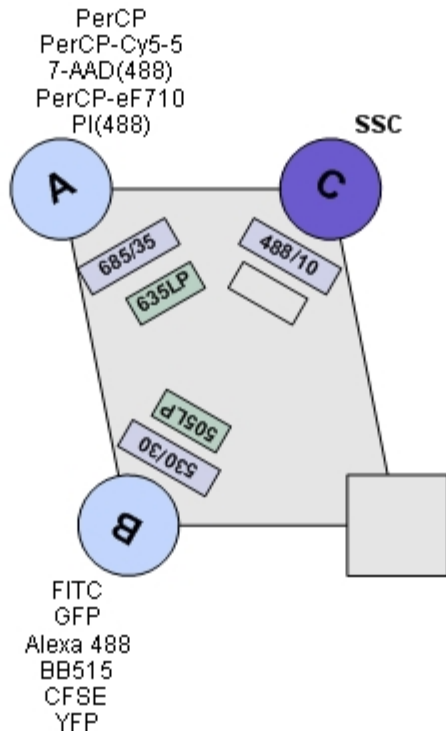

Violet Laser
(405nm)

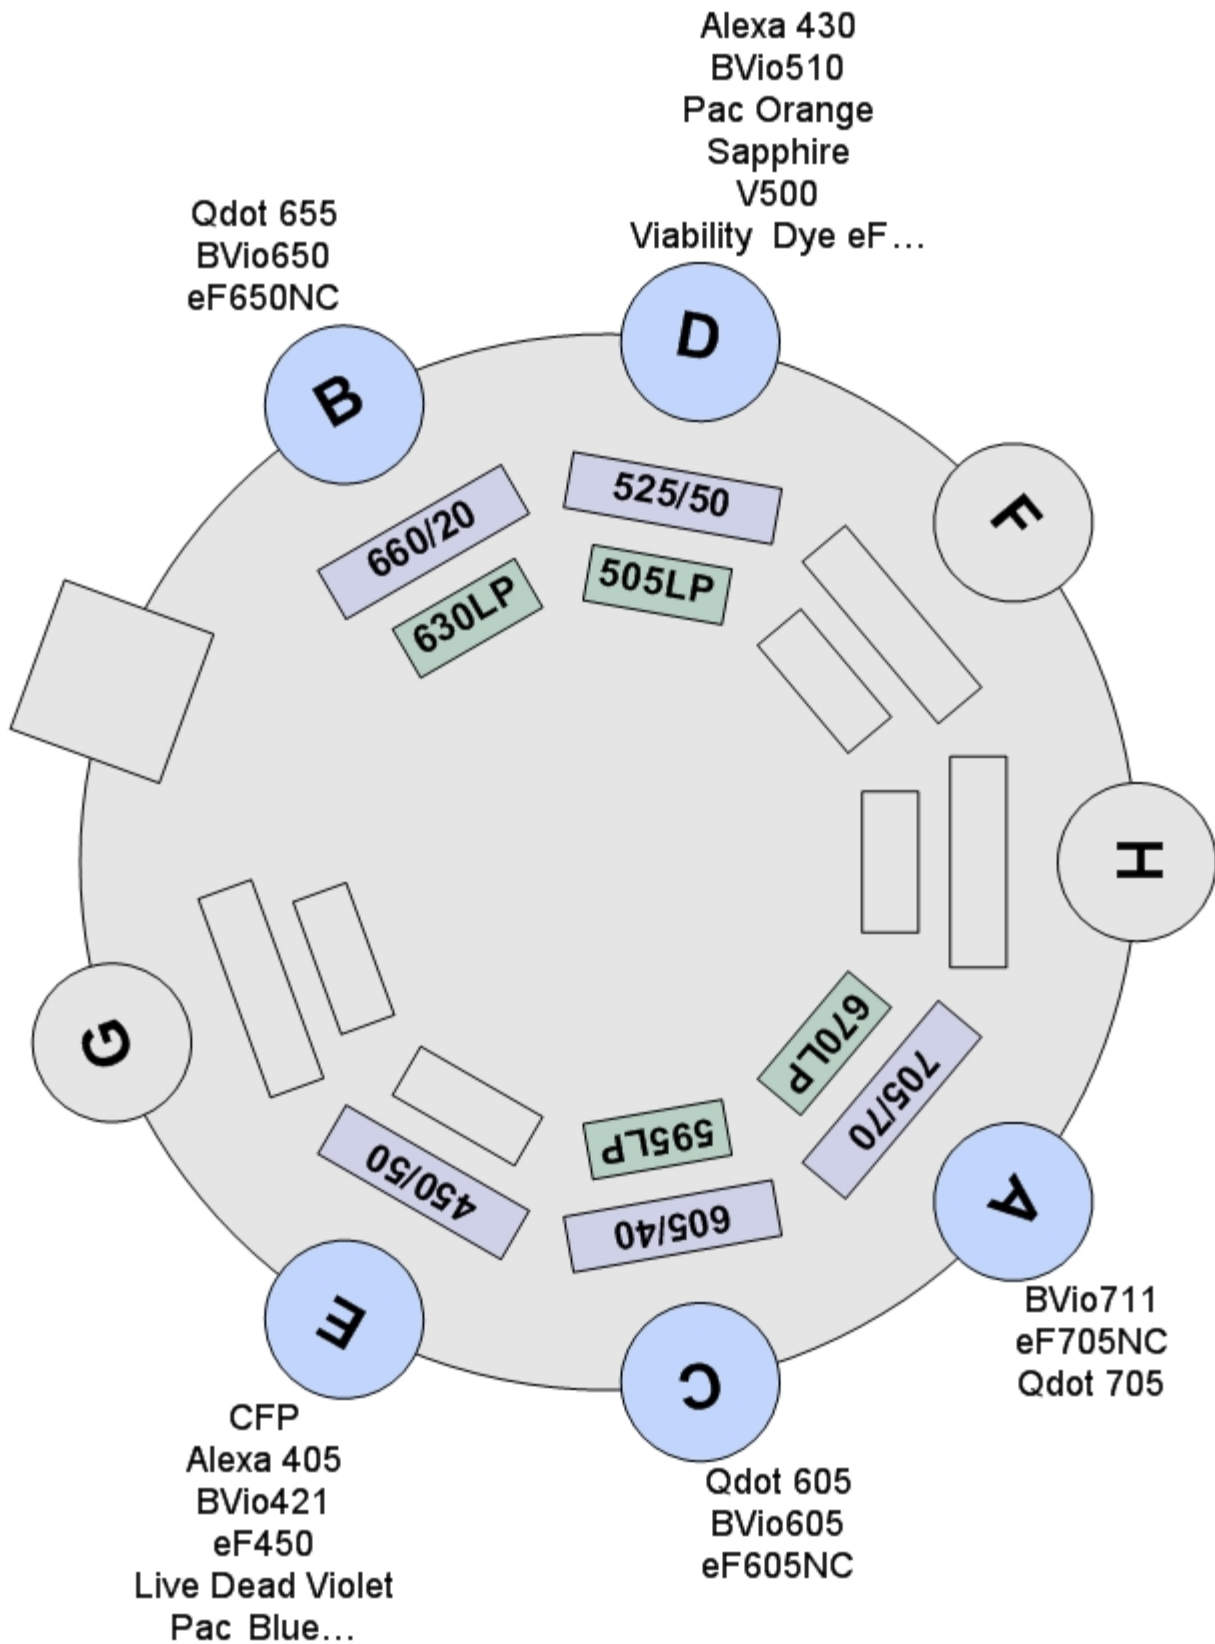

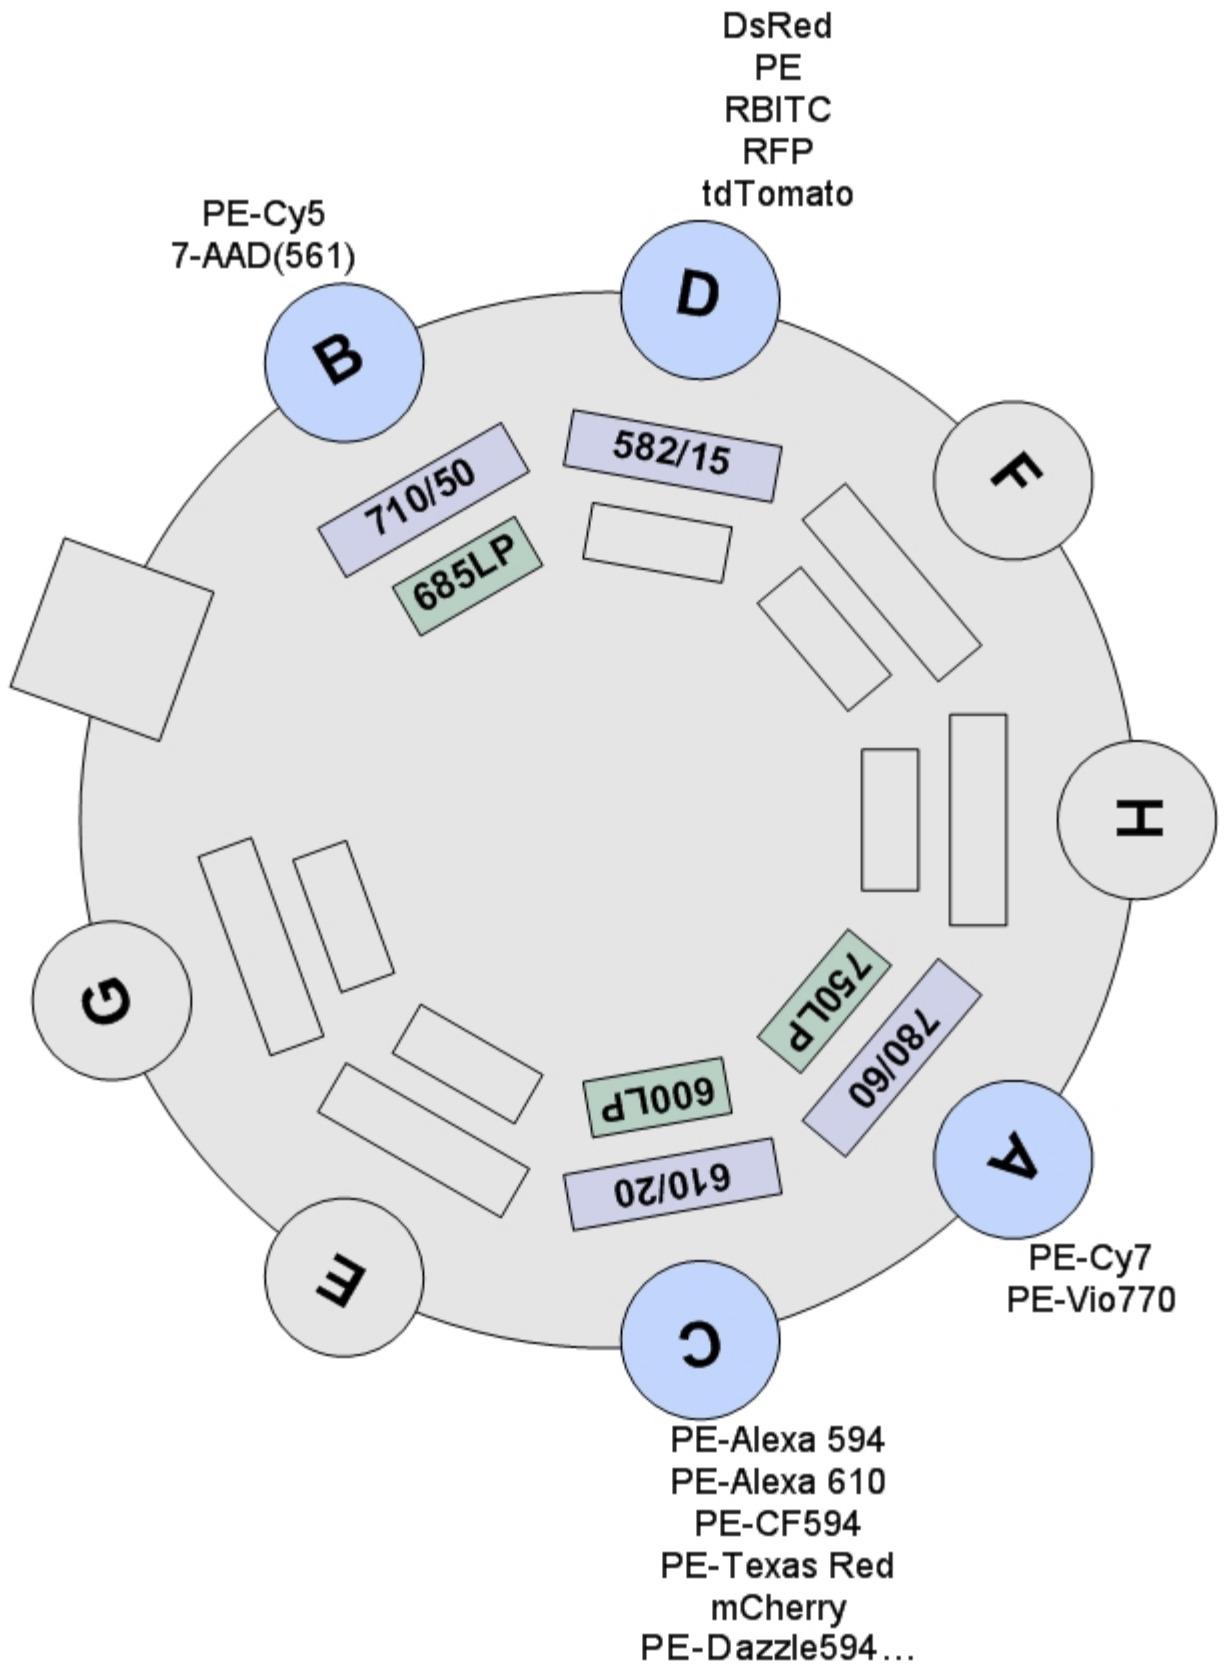

Comments:

Standardized Fluorochrome names

Blue A changed to 685/35 635LP

Y-G D changed to 582/15