


022217 LSRII-A 7B-2V-2UV-3R

Cytometer:
Cytometer Name:
Serial Number:
Input Device:
Window Extension:

LSRII
LSRII
1
Manual
10.00


User:
Institution:
Software:
Date:

EvanJellison
UCHC
BD FACSDiva 8.0.1
5/2/2017 4:47:42 PM

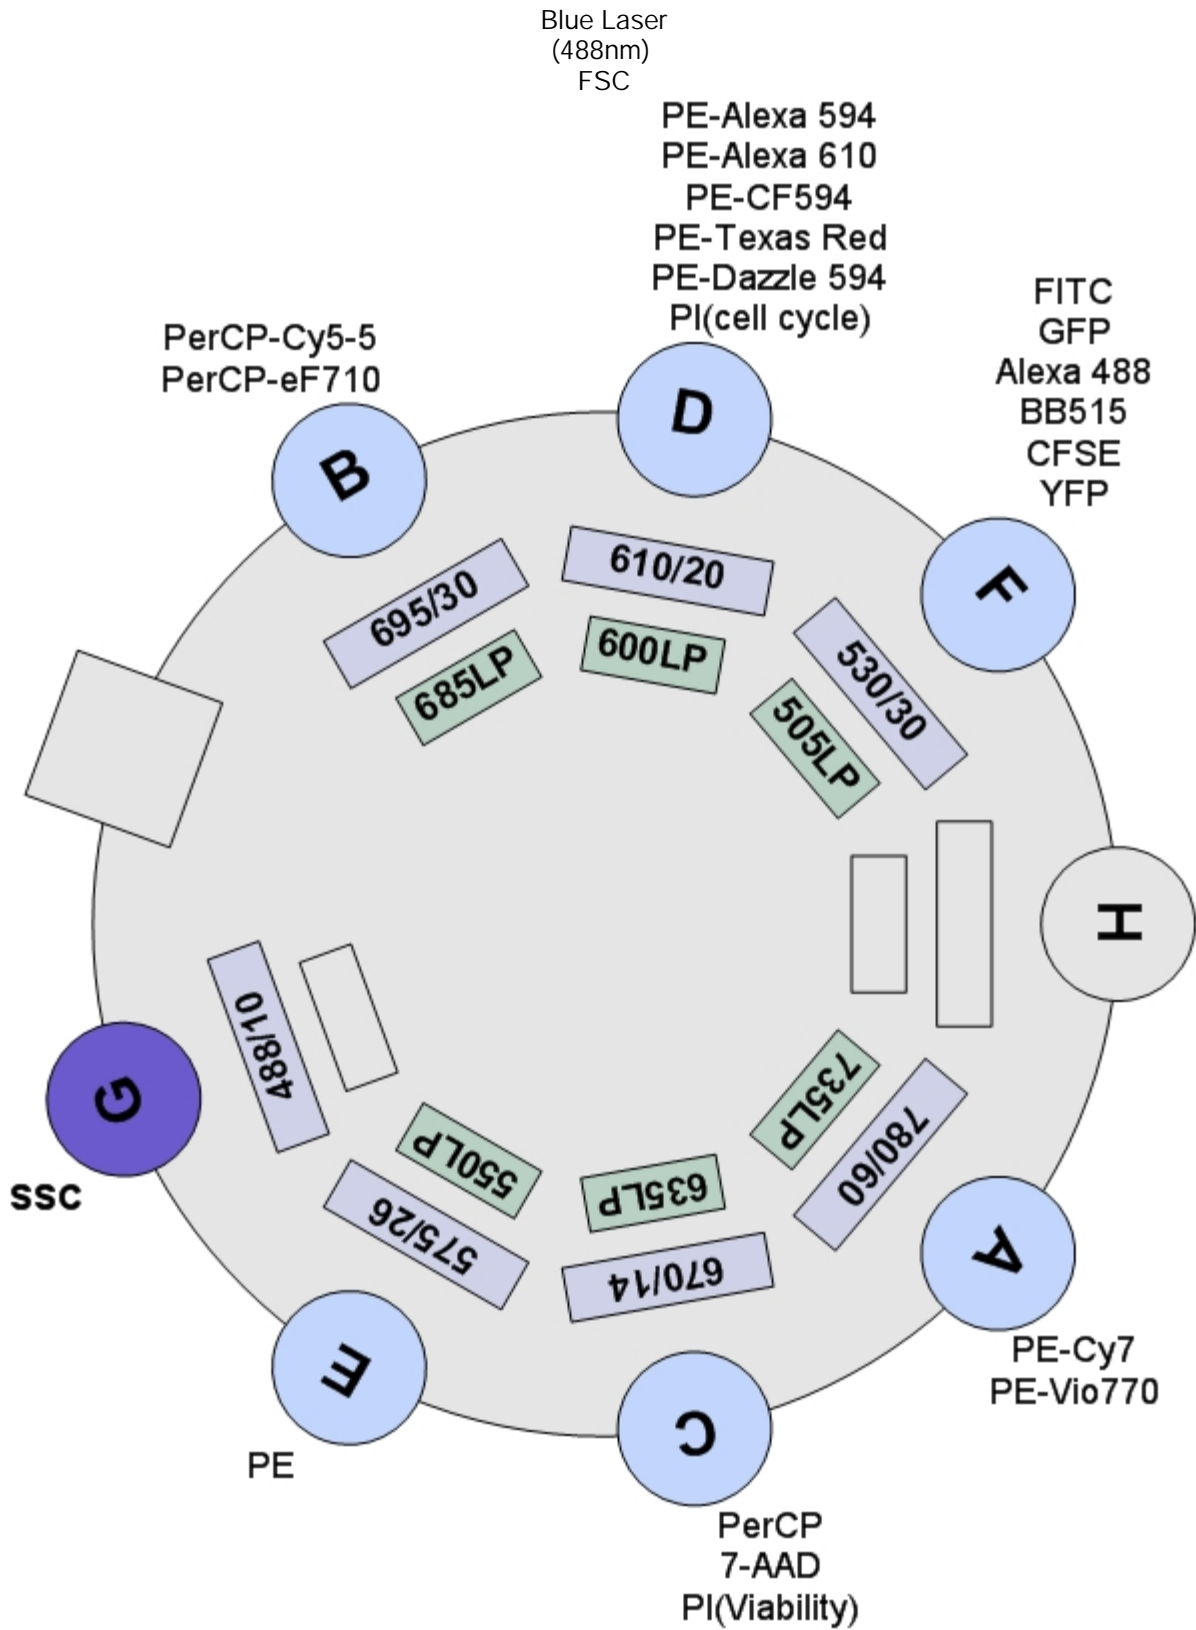

Violet Laser
(405nm)

Alexa 430
B Vio 510
Pac Orange
Sapphire
V500
Viability Dye eF...

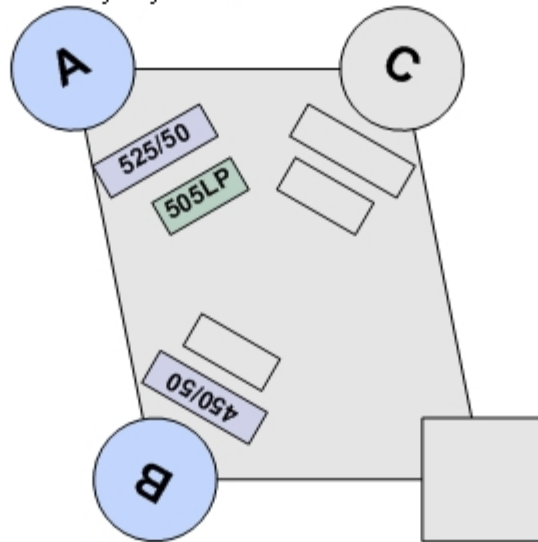


CFP
Alexa 405
B Vio 421
eF450
Live Dead Violet
Pac Blue...

Red Laser
(633nm)


APC-Cy7
APC-H7
APC-eF780
APC-Fire 750
Live Dead Near
IR

APC
Alexa 647
eF660
Live Dead Far
Red

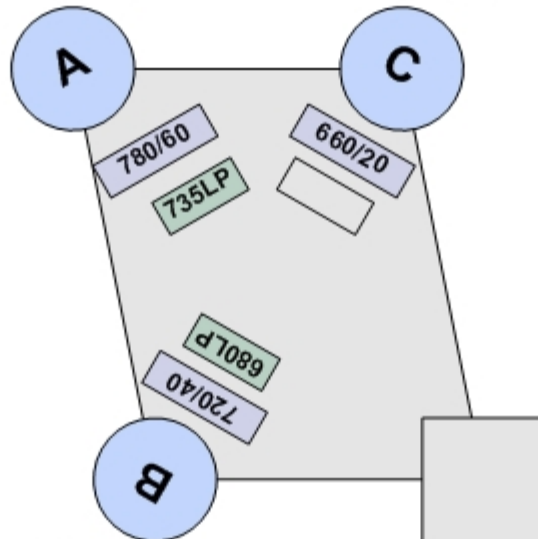

APC-R700
Alexa 700

355 UV Laser
(355nm)

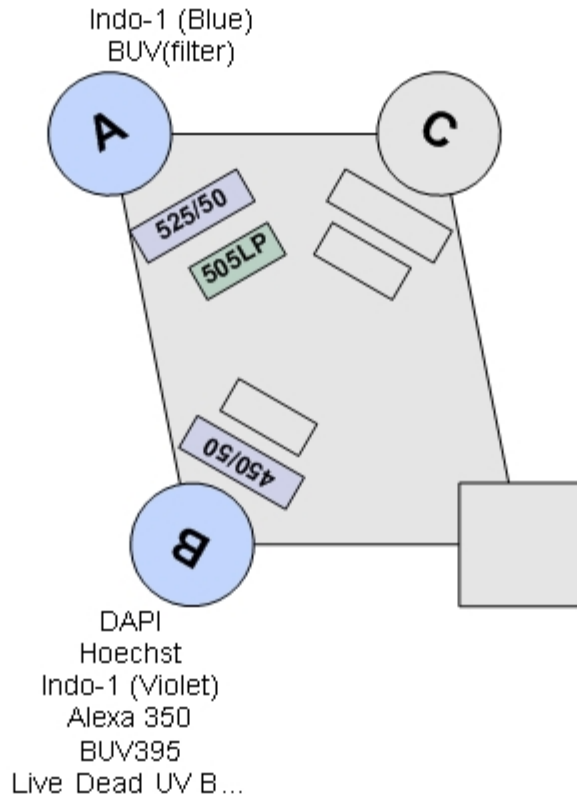

Comments:

Changed namers to reflect naming conventions

Actual Violet B 450/50, not 440/40 (BD)

Actual UV B 450/50, not 440/40 (BD)